




GOVERNMENT OF GILGIT- BALTISTAN
OFFICE OF THE MEDICAL SUPERINTENDENT
GILGIT CARDIAC HOSPITAL

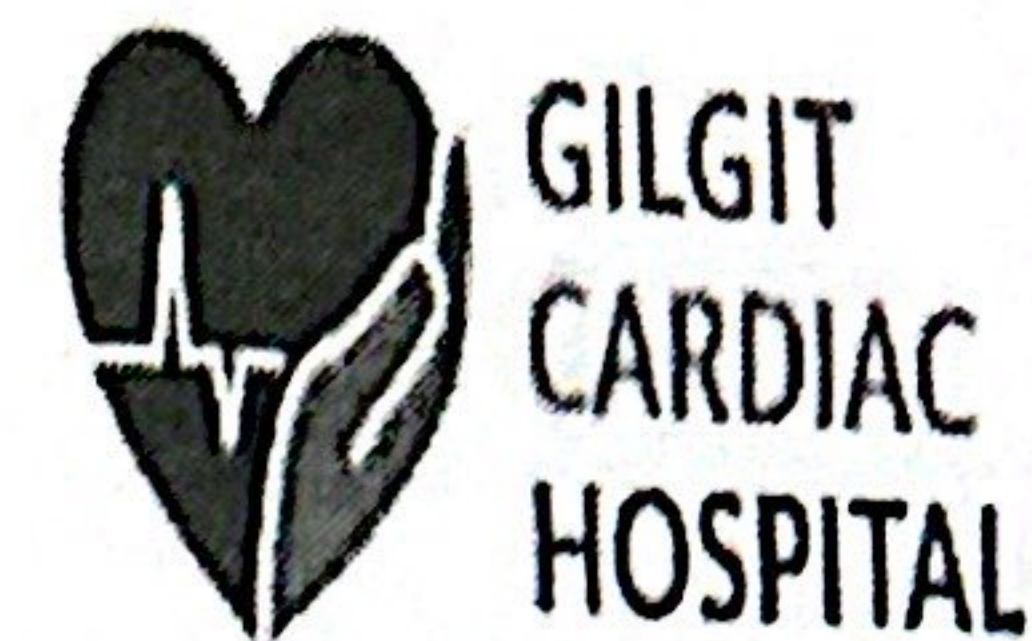


No.2507/GCH/Acct/2023

Dated ;04 August 2025

TENDER NOTICE

1. Sealed tenders are invited from firms/registered contractors for the repair/maintenance and supply/fixing of spare parts of government vehicles for the financial year 2025-26 for the office of the Medical Superintendent, Gilgit Cardiac Hospital.
2. Interested firms must deposit earnest money @ 2% of the bid amount in the form of a Call Deposit Receipt (CDR) from any scheduled bank, in favour of Medical Superintendent Gilgit Cardiac Hospital.
3. Sealed tenders must reach the office of the Medical Superintendent Gilgit Cardiac Hospital on or before 19th August 2025 at 11:00 AM. Tenders will be opened on the same day at 11:30 AM, in the presence of the bidders or their authorized representatives.
4. Conditional or incomplete tenders will be rejected.
5. Only registered firms/dealers are eligible to participate. A copy of registration must be attached; otherwise, the tender will be rejected.
6. The quantity of work may be increased or decreased as per the hospital's requirements.
7. Bidders may obtain a complete set of bidding documents along with evaluation criteria from the hospital office by submitting a non-refundable fee of Rs. 2,000/- (original receipt) at Gilgit Cardiac Hospital, Near Lalik Jan Stadium, Main Public Chowk, Jutial, Gilgit.
8. The office reserves the right to accept or reject any or all bids as per PPRA Rules.
9. Only computerized rates will be accepted.
10. The Medical Superintendent, Gilgit Cardiac Hospital, reserves the right to cancel or postpone the tender at any time.
11. If any items are not listed in the tender document and are required in the future, the vendor will be responsible to supply them as per prevailing market rates.
12. The accepted tender rates shall remain applicable for the entire financial year 2025-26.

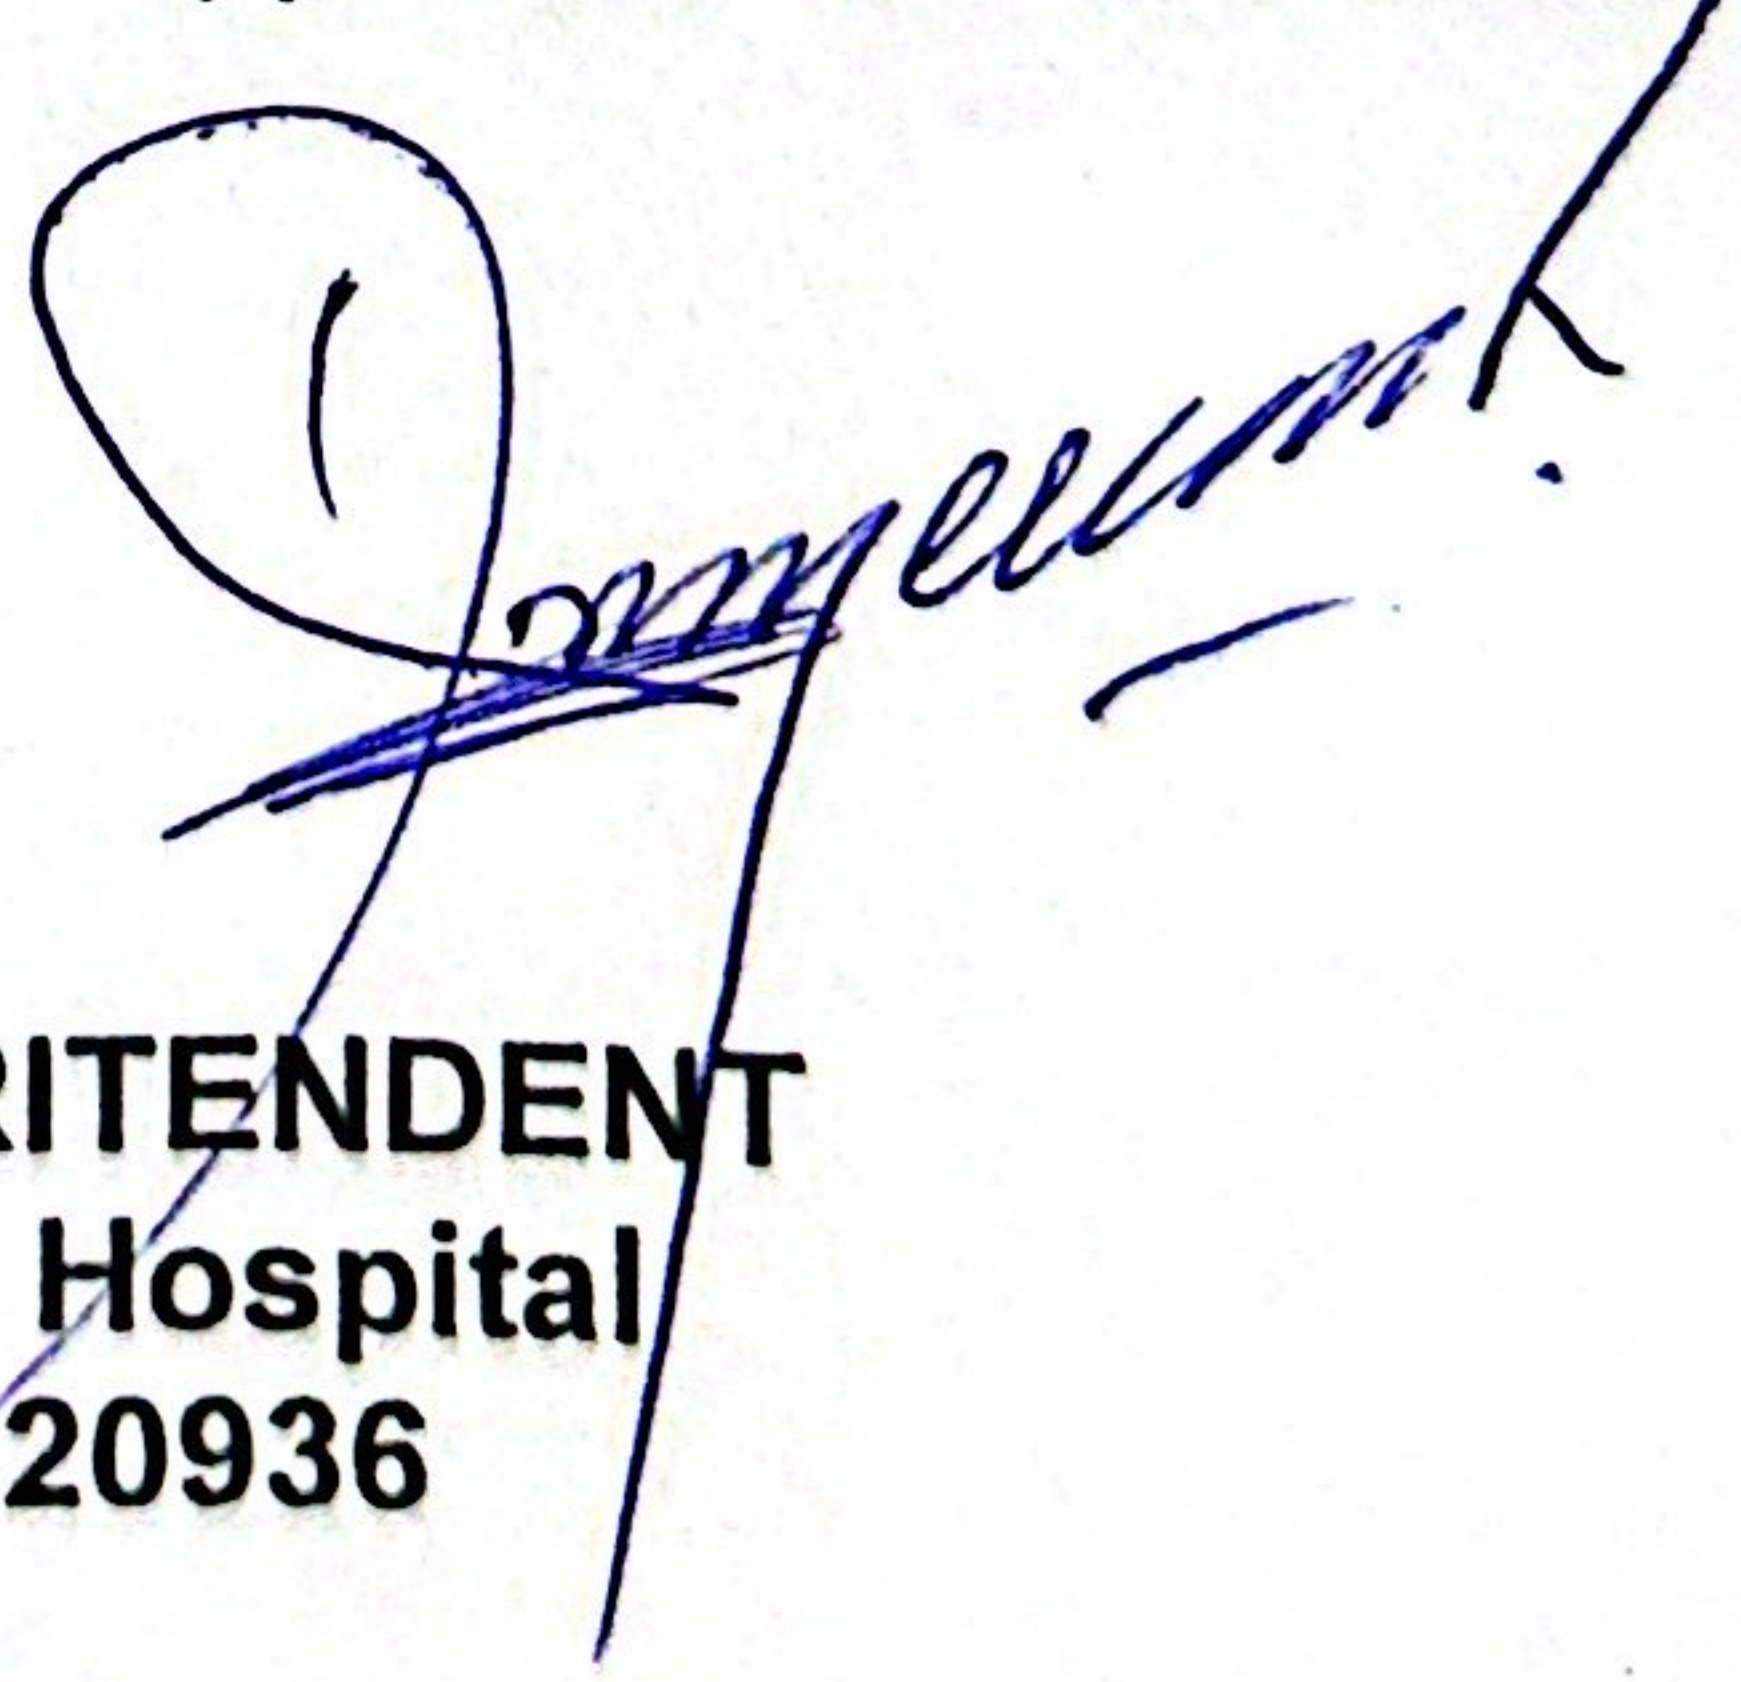
MEDICAL SUPERITENDENT
Gilgit Cardiac Hospital
Ph#05811-920936